



A Ostlund  
Ekelidsvagen, 5  
S 45740, Fjallbacka  
Sweden

15 October 2019

**Rif.CEDAD: 2019\_0165**

### **Results of Radiocarbon Dating**

Dear sir, please find enclosed the results of the radiocarbon dating of the samples you submitted to CEDAD (AMS and radiocarbon dating facility, University of Lecce, Italy) and listed in Table 1.

<b>Sample ID</b>	<b>CEDAD Code</b>	<b>Provenience</b>
20 prov 7	LTL19687A	
16 prov 9	LTL19688A	
19 prov 6	LTL19689A	
16 prov 10	LTL19690A	
20 prov 8	LTL19691A	
19 prov 5	LTL19692A	

TABLE 1. SUMMARY OF THE DATED SAMPLES.

Macro contaminants were removed from the samples by mechanical handpicking under optical microscope. The selected portion of the samples was treated in order to chemically remove any possible source of contamination.

The purified sample material was then converted to carbon dioxide by combustion in sealed quartz tubes. The obtained carbon dioxide was converted at 550°C into graphite by using ultrahigh purity Hydrogen as reducing medium and 2 mg iron powder as catalyst.



The sample yielded enough graphite to allow an accurate determination of the radiocarbon age by the accelerator mass spectrometer.

The radiocarbon concentrations have been determined in the accelerator mass spectrometer by comparing the  $^{12}\text{C}$ ,  $^{13}\text{C}$  currents and the  $^{14}\text{C}$  counts obtained from the samples with those obtained from standard materials supplied by IAEA (International Atomic Energy Agency) and NIST (National Institute of Standard and Technology).

The "conventional radiocarbon age" was calculated with a  $\delta^{13}\text{C}$  correction based on the  $^{13}\text{C}/^{12}\text{C}$  ratio measured directly with the accelerator. For the estimation of the measurement uncertainty (standard deviation) both the radioisotope counting statistics and the scattering of the data have been taken into account. The larger of the two is given as final error in Table 2.

Sample	Radiocarbon Age (BP)	$\delta^{13}\text{C}$ (‰) <sup>(**)</sup>	Note
LTL19687A	640 ± 45	-24.2 ± 0.6	
LTL19688A	352 ± 45	-30.9 ± 0.2	
LTL19689A	555 ± 45	-26.2 ± 0.5	
LTL19690A	521 ± 45	-26.2 ± 0.4	
LTL19691A	774 ± 45	-28.3 ± 0.2	
LTL19692A	365 ± 45	-27.1 ± 0.4	

(\*\*) The listed values of the carbon stable isotopes fractionation term ( $\delta^{13}\text{C}$ ) are measured by AMS. These values can differ from the natural fractionation and from those measured by IRMS.

TABLE 2. MEASURED VALUES.

The conventional radiocarbon ages of the samples were converted into calendar years by using the software OxCal Ver. 3.5 based on the last atmospheric dataset [Reimer PJ, et al. 2013 *Radiocarbon* 55 No. 4-1869-1887]. The results of the calibration are reported in the following figures.



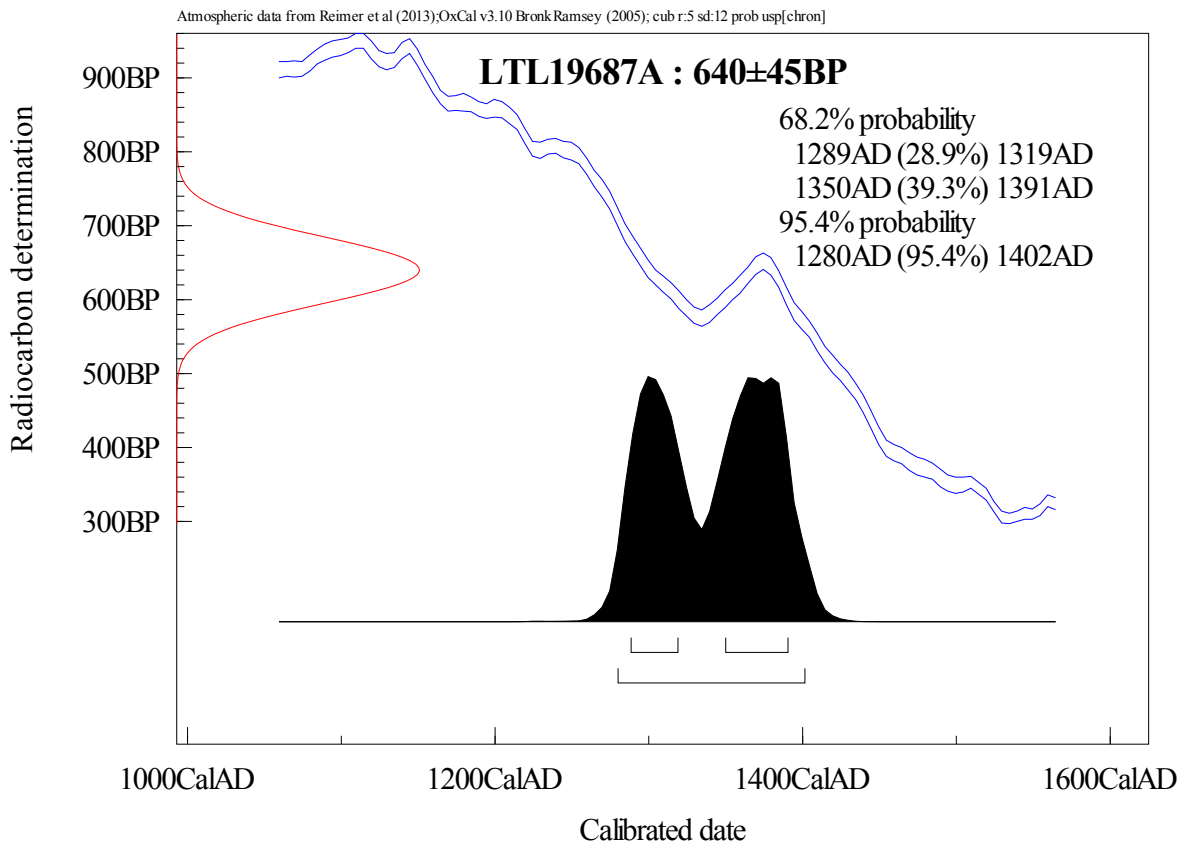



Figure 1. Calibration of the radiocarbon age of the sample LTL19687A.

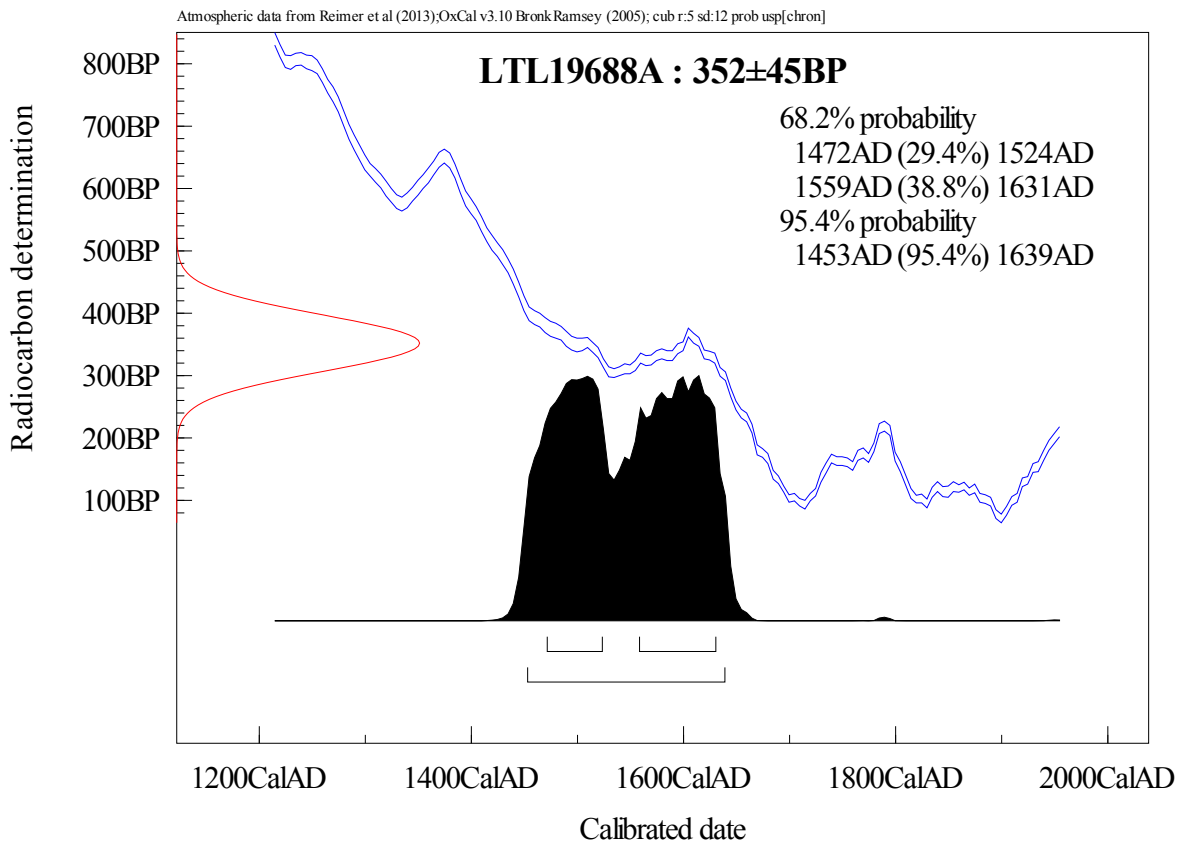


**Figure 2. Calibration of the radiocarbon age of the sample LTL19688A.**

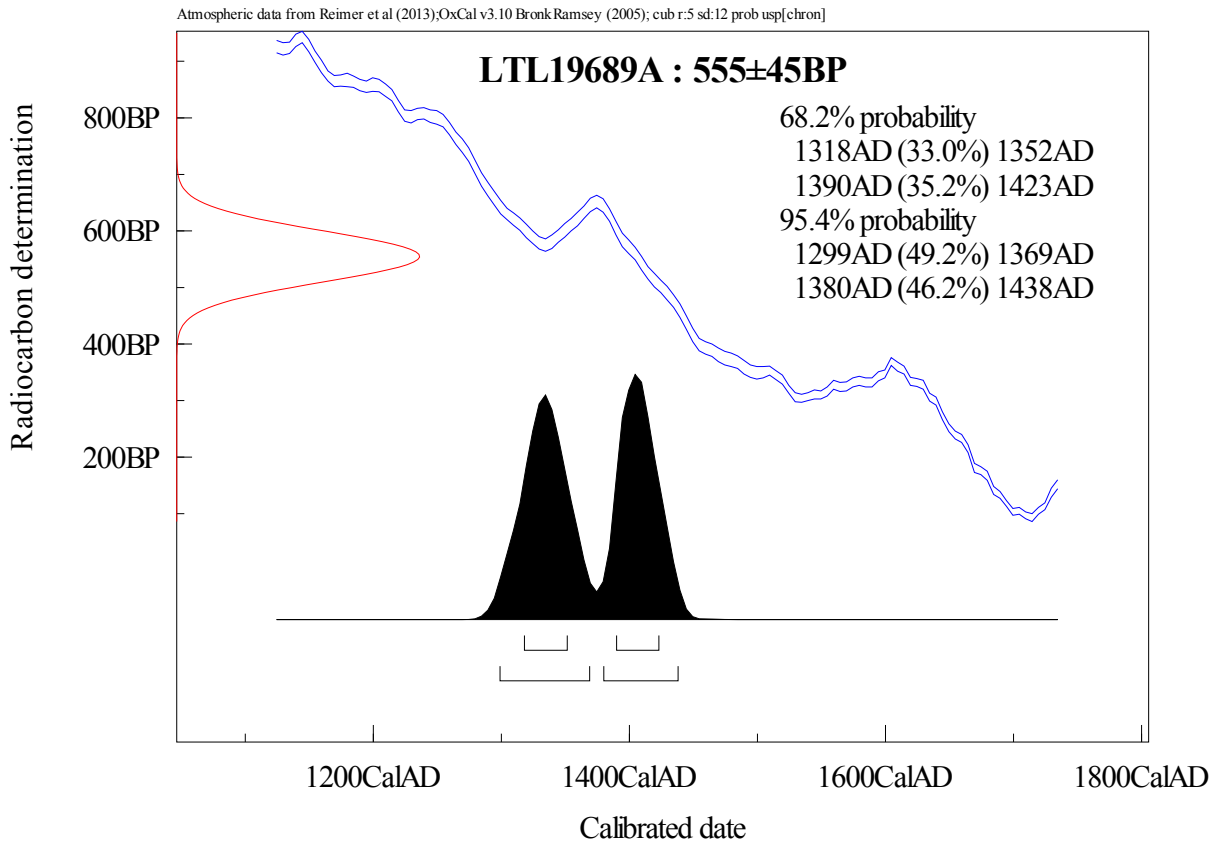


**Figure 3. Calibration of the radiocarbon age of the sample LTL19689A.**

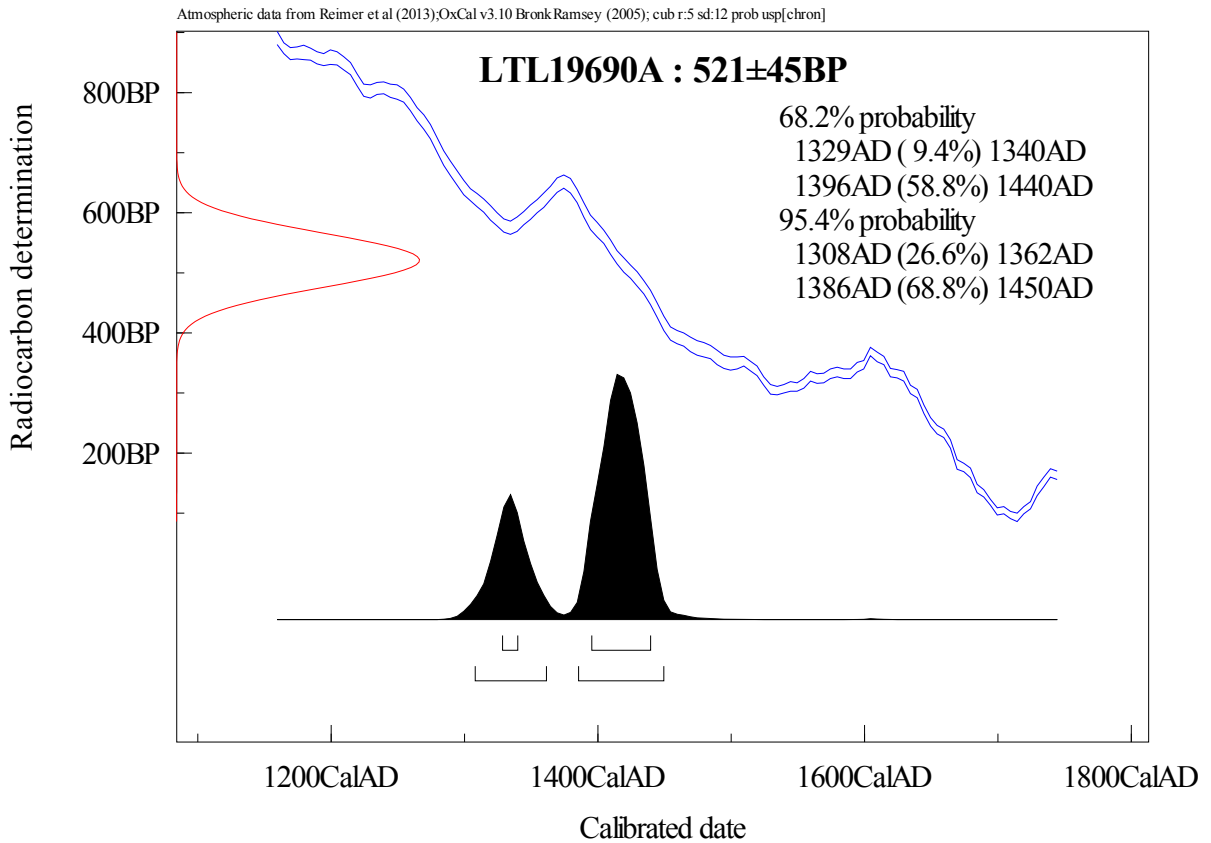

**Figure 4. Calibration of the radiocarbon age of the sample LTL19690A.**

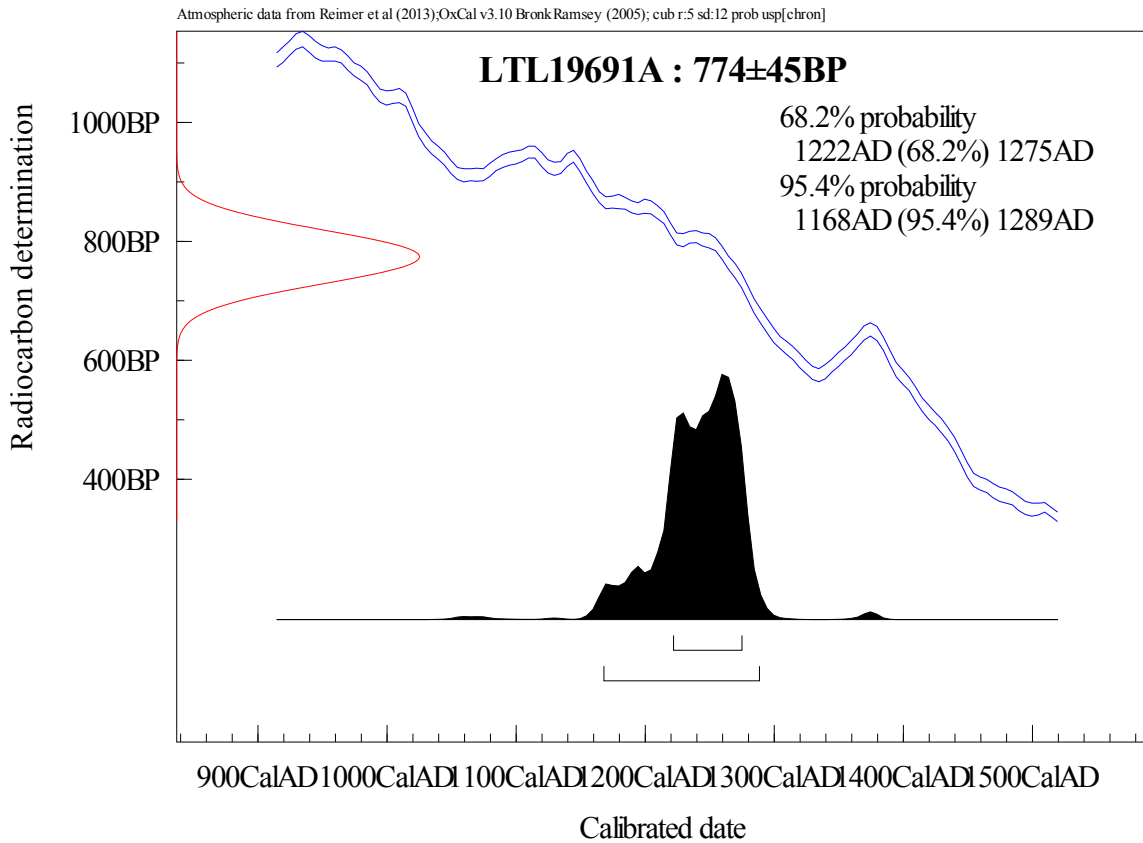

**Figure 5. Calibration of the radiocarbon age of the sample LTL19691A.**

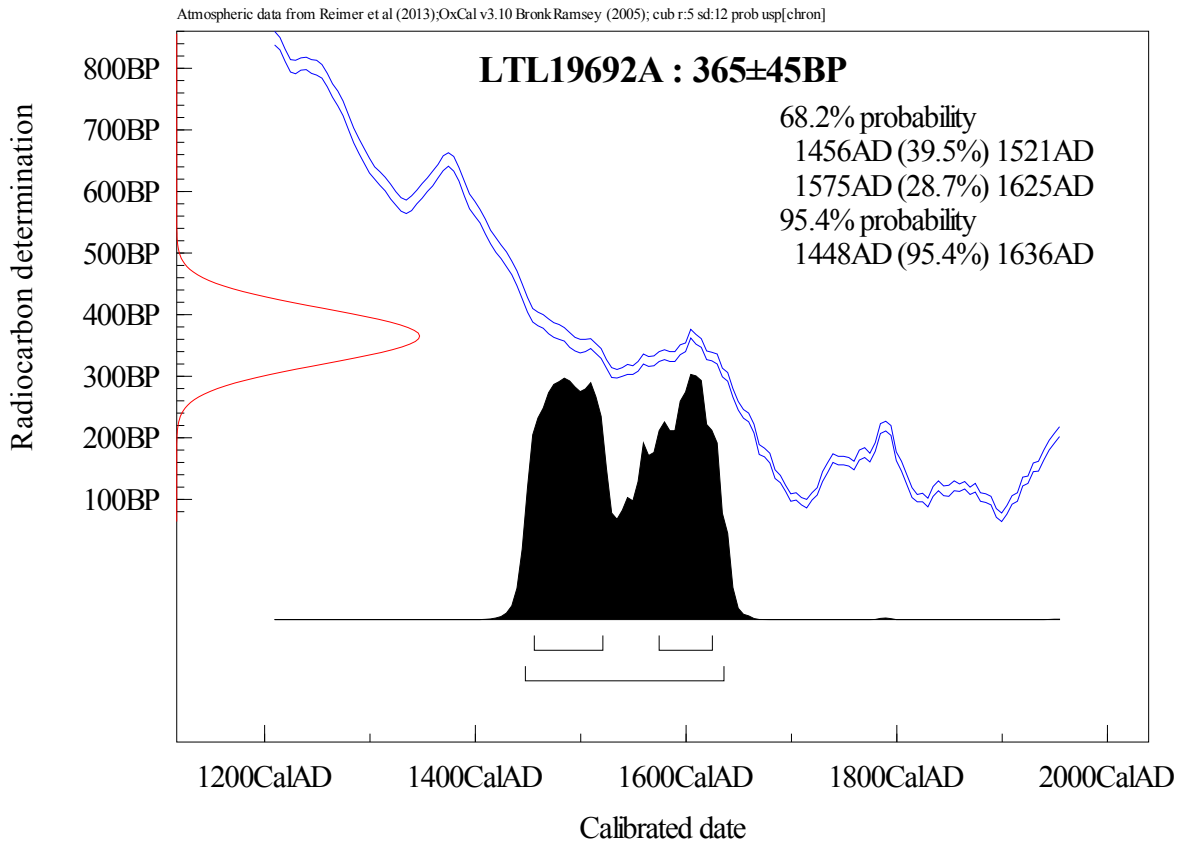

**Figure 6. Calibration of the radiocarbon age of the sample LTL1962A.**

Best Regards,

Prof. Dr. Lucio Calcagnile

Director, Centro di Datazione e Diagnostica dell'Università del Salento