



TABLE 1. SUMMARY OF THE DATED SAMPLES.

Dr. Stig Swedberg
Rio Kulturkooperativ
Sweden

31 July 2018

Rif.CEDAD: 2018_0138_mod

Results of Radiocarbon Dating

Dear sir, please find enclosed the results of the radiocarbon dating of the samples you submitted to CEDAD (AMS and radiocarbon dating facility, University of Lecce, Italy) and listed in Table 1.

<i>Sample ID</i>	<i>CEDAD Code</i>	<i>Provenance</i>
S 17 066 005	LTL18119A	
S 17 066 006	LTL18120A	
S 17 066 007	LTL18121A	
S 17 066 008	LTL18122A	
S 17 066 009	LTL18123A	

Macro contaminants were removed from the samples by mechanical handpicking under optical microscope. The selected portion of the samples was treated in order to chemically remove any possible source of contamination.

The purified sample material was then converted to carbon dioxide by combustion in sealed quartz tubes. The obtained carbon dioxide was converted at 550°C into graphite by using ultrahigh purity Hydrogen as reducing medium and 2 mg iron powder as catalyst. The sample yielded enough graphite to allow an accurate determination of the radiocarbon age by the accelerator mass spectrometer.



TABLE 2. MEASURED VALUES.

The radiocarbon concentrations have been determined in the accelerator mass spectrometer by comparing the ^{12}C , ^{13}C currents and the ^{14}C counts obtained from the samples with those obtained from standard materials supplied by IAEA (International Atomic Energy Agency) and NIST (National Institute of Standard and Technology).

The "conventional radiocarbon age" was calculated with a $\delta^{13}\text{C}$ correction based on the $^{13}\text{C}/^{12}\text{C}$ ratio measured directly with the accelerator. For the estimation of the measurement uncertainty (standard deviation) both the radioisotope counting statistics and the scattering of the data have been taken into account. The larger of the two is given as final error in Table 2.

Sample	Radiocarbon Age (BP)	$\delta^{13}\text{C}$ (‰) ^(**)	Note
LTL18119A	2030 ± 25	-20.7 ± 0.5	
LTL18120A	2151 ± 25	-18.5 ± 0.5	
LTL18121A	2398 ± 35	-23.2 ± 0.6	
LTL18122A	2202 ± 25	-24 ± 0.7	
LTL18123A	1748 ± 25	-19.6 ± 0.4	

(**) The listed values of the carbon stable isotopes fractionation term ($\delta^{13}\text{C}$) are measured by AMS. These values can differ from the natural fractionation and from those measured by IRMS.

The conventional radiocarbon ages of the samples were converted into calendar years by using the software OxCal Ver. 3.5 based on the last atmospheric dataset [Reimer PJ, et al. 2013 *Radiocarbon* 55 No. 4-1869-1887]. The results of the calibration are reported in the following figures.

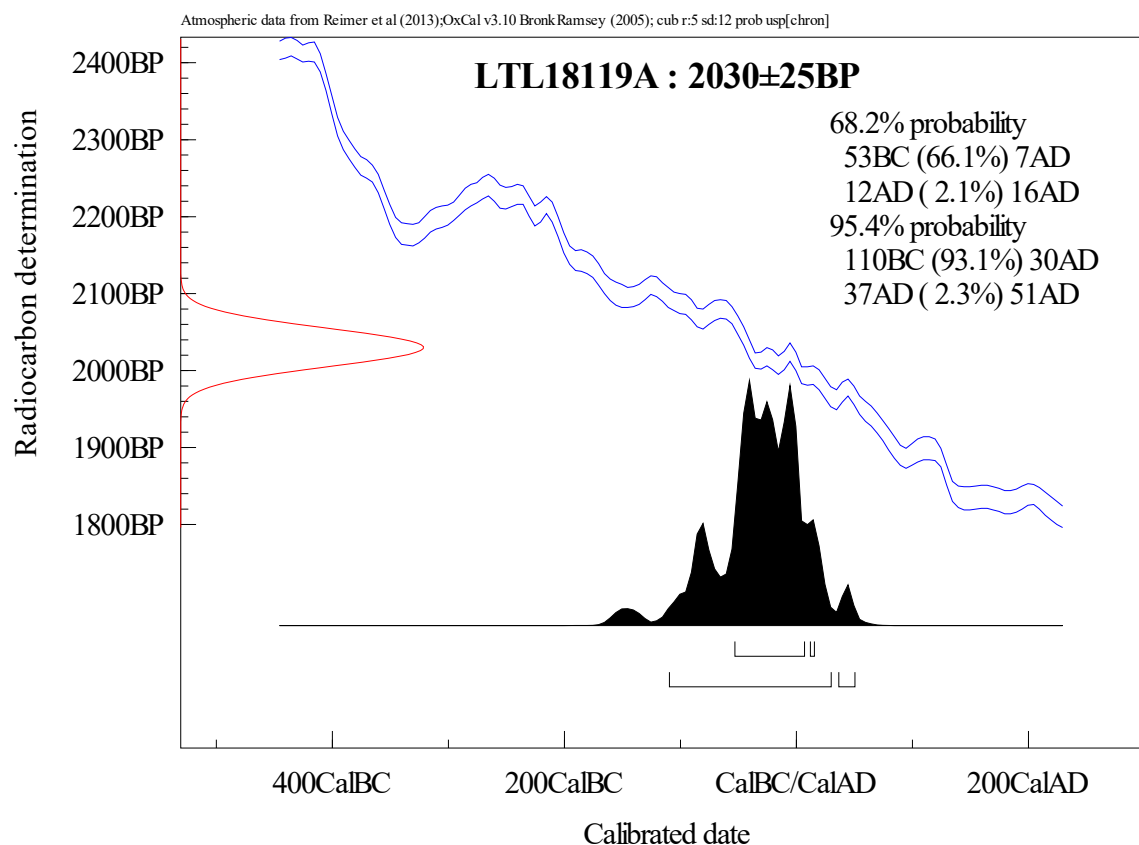


Figure 1. Calibration of the radiocarbon age of the sample LTL18119A.

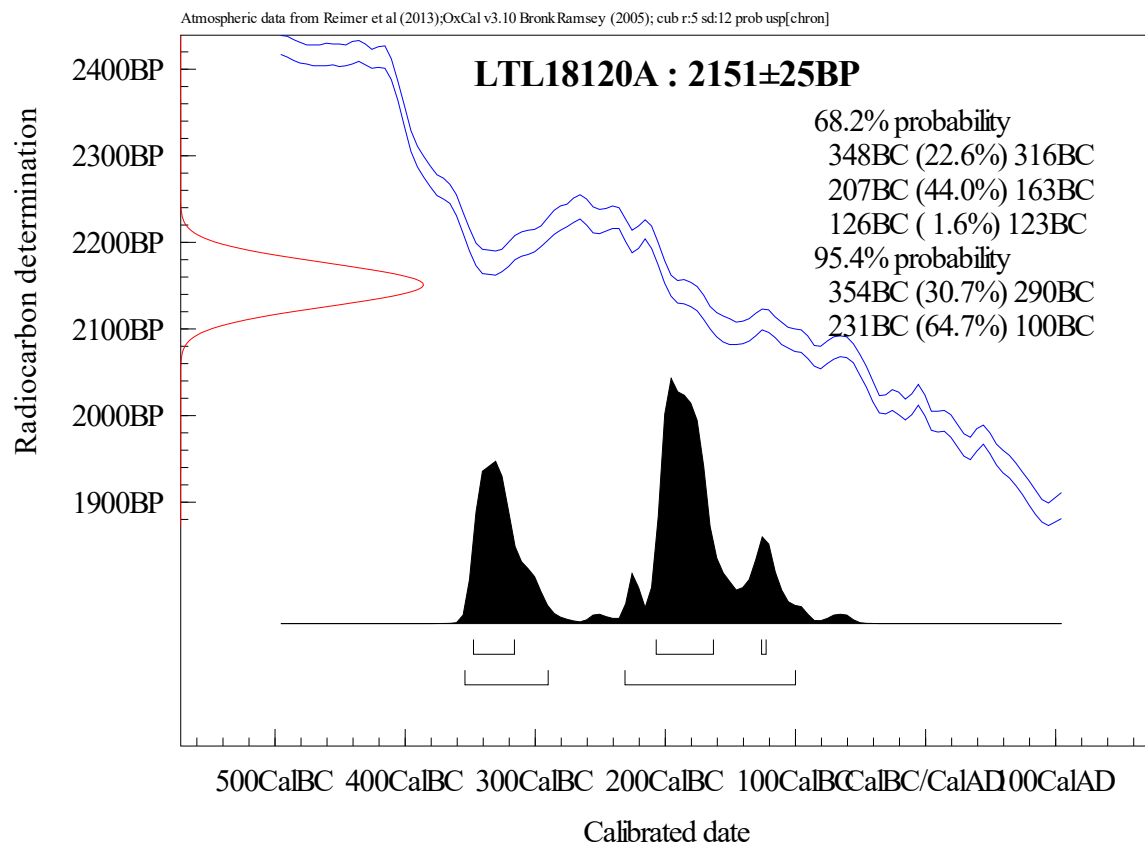


Figure 2. Calibration of the radiocarbon age of the sample LTL18120A.

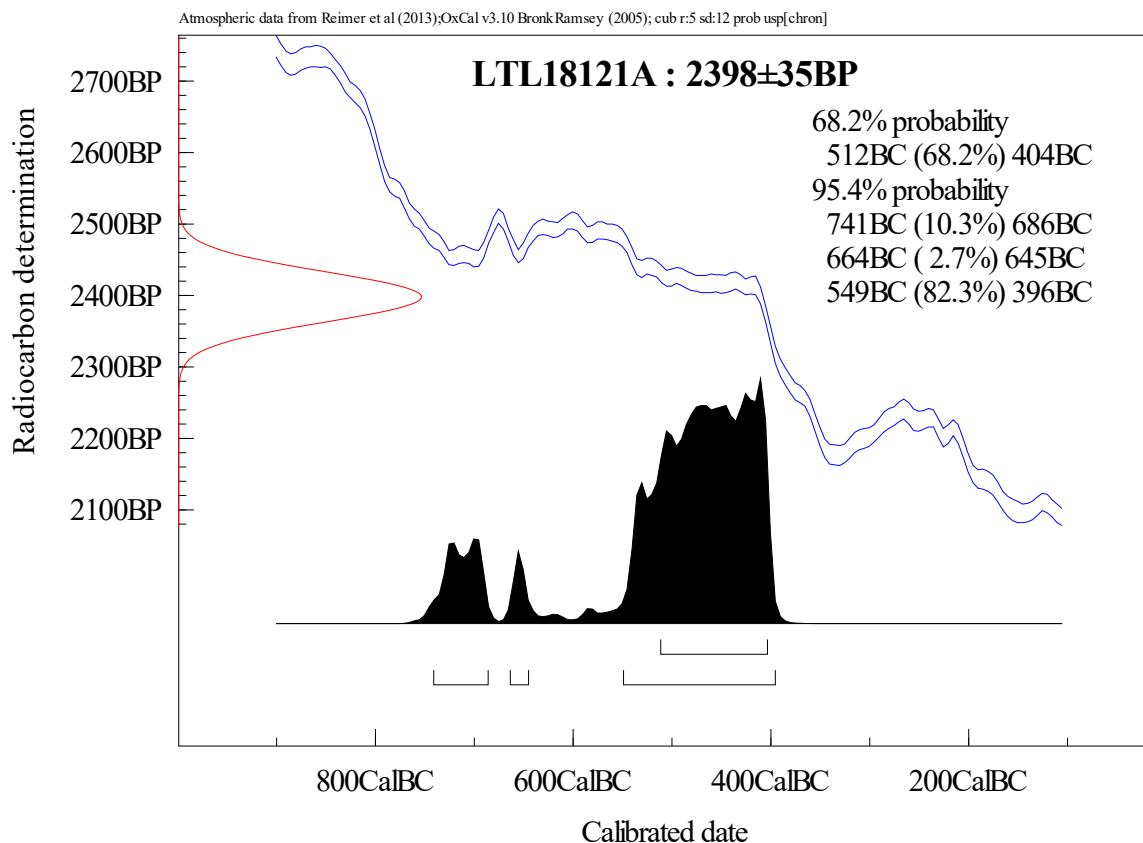
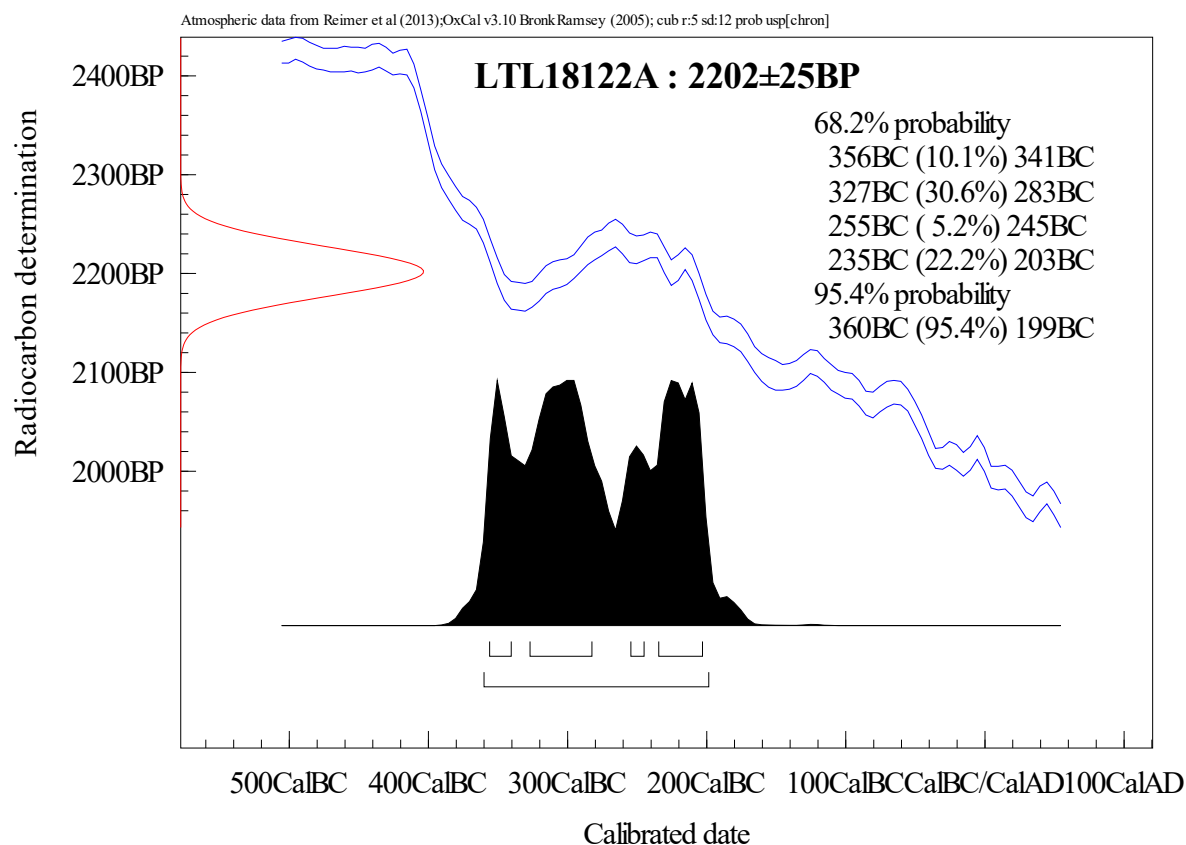


Figure 3. Calibration of the radiocarbon age of the sample LTL18121A.



**Figure 4. Calibration of the radiocarbon age of the sample
LTL18122A.**

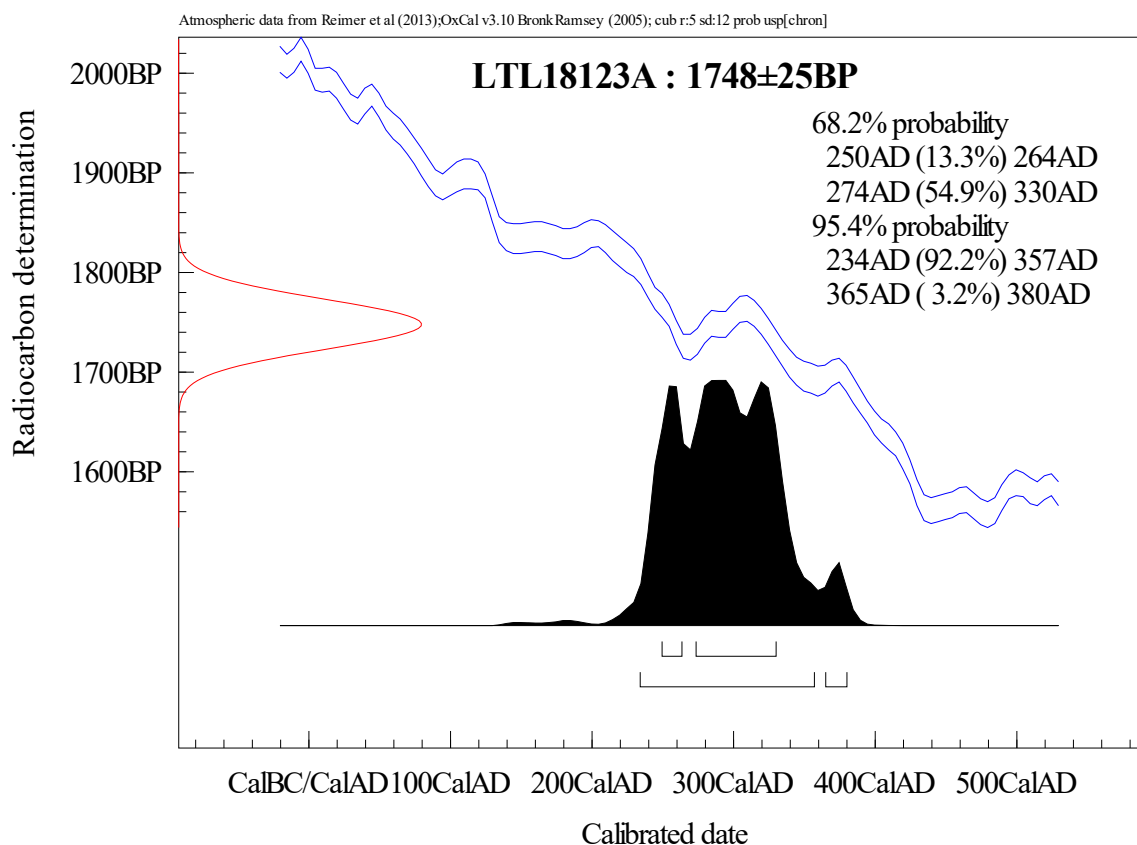


Figure 5. Calibration of the radiocarbon age of the sample LTL18123A.

Best Regards,

Prof. Dr. Lucio Calcagnile

Director, Centro di Datazione e Diagnostica dell'Università del Salento